VERIFICATION OF CALIBRATION REPORT
of DataMaster dmt Breath Test Instrument
State of Alaska

Serial #: 100421   **Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program**   Date: 10/14/2011

External Standard Test Values

```
EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.35: 0.078
LOT #: 07511080A1
EXPIRATION: 03/01/2013

BLANK TEST              0.000   16:23
INTERNAL STANDARD     VERIFIED  16:23
EXTERNAL STANDARD       0.079   16:23
BLANK TEST              0.000   16:24
EXTERNAL STANDARD       0.079   16:24
BLANK TEST              0.000   16:25
EXTERNAL STANDARD       0.079   16:25
BLANK TEST              0.000   16:26
EXTERNAL STANDARD       0.079   16:26
BLANK TEST              0.000   16:27
EXTERNAL STANDARD       0.079   16:28
BLANK TEST              0.000   16:28

Average = 0.0790
Std Dev = 0.0000
```

Diagnostic Check

```
VERSIONS
DMT: 1.01
PIC: 3.02
Modem: 2.0
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.6°C        PASSED
Breath Tube    = 47.7°C        PASSED

PUMP INFO
Flow Rate = 4.591 L/M          PASSED

DETECTOR INFO
PUMP ON                        PASSED
PUMP OFF                       PASSED

FILTER INFO
Filter 1                       PASSED
Filter 2                       PASSED
Filter 3                       PASSED

INTERNAL STANDARD              PASSED
```
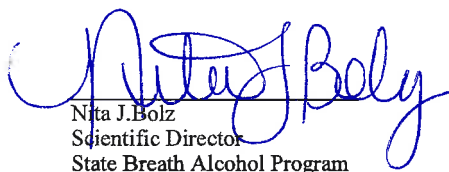
I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

(1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.

(2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.

(3) I am the Scientific Director of the State Breath Alcohol Program.

(4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.

(5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.

(6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz   11/9/11
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this ___9___ day of __Nov__, 20 _11_

Nikki Roth, Notary Public
My Commission Expires With Office